

## Mechanical Emergency Door Release

During a power failure, you will not be able to open the centrifuge lid with the regular electric lid release. A mechanical override is provided to allow sample recovery in the case of an emergency. However, this should be used only in emergencies and after the rotor has come to a complete stop.



**WARNING** The rotor can still be spinning at high speed. If touched, it can cause serious injuries.

Always wait 20 minutes until the rotor has come to a stop without braking. The brake does not work when there is no current. The braking process lasts much longer than usual.


Proceed as follows:

1. Make sure the rotor has stopped (view port in the lid).



**WARNING** Never use your hand or other tools to brake the rotor.

2. Pull out the power supply plug.
3. On the right side of the housing is one white plastic plug which you can pry out of the side plate with a screwdriver.  
Pull the release cord attached to it to trigger the mechanical door release. The door will open and the samples can be removed.

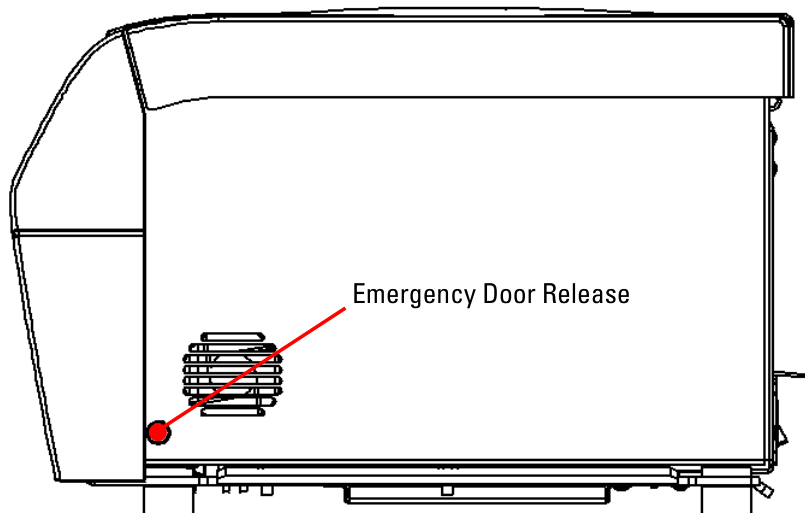

**Figure 5.** Emergency Door Release

4. Push the cord back into the centrifuge and mount the plug.

Reconnect the centrifuge once the power has been restored. Switch on the centrifuge. Press the OPEN key to have the door locks operative again.